


# AMICO BABY LDR UNIT (28x26x17)

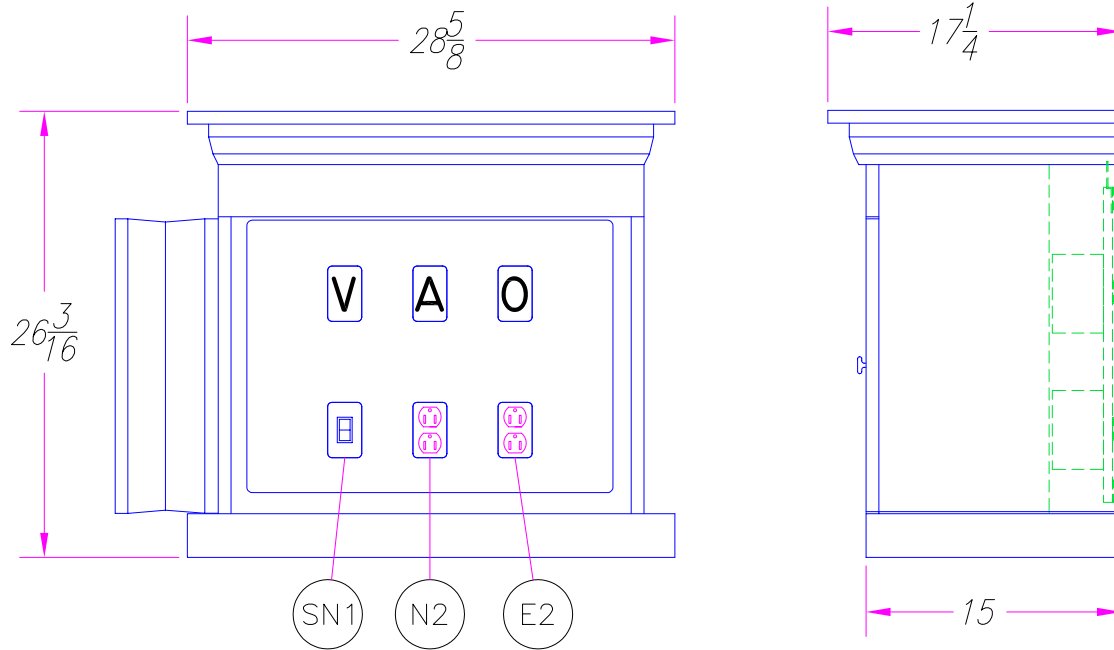

SYMBOL	QTY.	DESCRIPTION
N2	1	DUPLEX RECEPTACLE- NORMAL
E2	1	DUPLEX RECEPTACLE - RED
SN1	1	SWITCH , SP, 120V
A	1	GAS, AIR
V	1	GAS, VACUUM
O	1	GAS, OXYGEN

IMPORTANT: PLEASE VERIFY THAT THE ABOVE INFORMATIONS ARE CORRECT, AND SUPPLY THE REMAINING INFORMATIONS.

APPROVAL SIGNATURE \_\_\_\_\_

DATE \_\_\_\_\_

PHONE NO. \_\_\_\_\_

**AMICO Corporation**  
 21-121 Granton Drive  
 Richmond Hill, Ontario  
 L4B 3N4, CANADA  
 Tel: (905) 764-0800  
 Fax: (905) 764-0862  
 www.amico.com

HOSPITAL \_\_\_\_\_

LOCATION \_\_\_\_\_

QTY. (\_\_\_\_\_) TYPE \_\_\_\_\_ UNITS AS SHOWN / (\_\_\_\_\_) TYPE \_\_\_\_\_ UNITS OPPOSITE

**TYPICAL DRAWING**

A. NURSE CALL MFGR: \_\_\_\_\_ MODEL NO.: \_\_\_\_\_

B. MEDICAL GAS MFGR.: AMICO TYPE CONNECTION: \_\_\_\_\_

C. FINISH: \_\_\_\_\_ CEILING HEIGHT: \_\_\_\_\_

DRWG. NO.  
030124-C08

DRAWN BY: CE

CHECKED: CS

REV. NO.

DATE: 01/24/03